



**University of
Zurich**^{UZH}

**Zurich Open Repository and
Archive**

University of Zurich
University Library
Strickhofstrasse 39
CH-8057 Zurich
www.zora.uzh.ch

Year: 2021

Whole-body parametric [18 F]-FDG PET/CT improves interpretation of a distant lesion as venous embolus in a lung cancer patient

Messerli, Michael ; Kotasidis, Fotis ; Ferraro, Daniela A ; Kudura, Ken ; Treyer, Valerie ; Trinckauf, Josephine ; Weyermann, Corina ; Hüllner, Martin ; Kaufmann, Philipp ; Burger, Irene A

DOI: <https://doi.org/10.1007/s00259-020-05176-0>

Posted at the Zurich Open Repository and Archive, University of Zurich

ZORA URL: <https://doi.org/10.5167/uzh-200720>

Journal Article

Published Version



The following work is licensed under a Creative Commons: Attribution 4.0 International (CC BY 4.0) License.

Originally published at:

Messerli, Michael; Kotasidis, Fotis; Ferraro, Daniela A; Kudura, Ken; Treyer, Valerie; Trinckauf, Josephine; Weyermann, Corina; Hüllner, Martin; Kaufmann, Philipp; Burger, Irene A (2021). Whole-body parametric [18 F]-FDG PET/CT improves interpretation of a distant lesion as venous embolus in a lung cancer patient. *European Journal of Nuclear Medicine and Molecular Imaging*, 48(6):2047-2048.

DOI: <https://doi.org/10.1007/s00259-020-05176-0>



Whole-body parametric [^{18}F]-FDG PET/CT improves interpretation of a distant lesion as venous embolus in a lung cancer patient

Michael Messerli¹ · Fotis Kotasidis² · Daniela A. Ferraro¹ · Ken Kudura¹ · Valerie Treyer¹ · Josephine Trinckauf¹ · Corina Weyermann¹ · Martin Hüllner¹ · Philipp Kaufmann¹ · Irene A. Burger^{1,3} 

Received: 7 September 2020 / Accepted: 20 December 2020
© The Author(s) 2021

Despite well-known limitations of static analysis of FDG-PET images, the ease of its use leads to a widespread use of semi-quantitative indices, most commonly the standardized uptake value (SUV). In contrast to static imaging, dynamic imaging with kinetic modeling allows estimation of quantitative parameters, independent of uptake time, body weight, or injected dose, therefore potentially improving the interpretation of FDG-accumulation [1]. With improvements in scanner sensitivity and reconstruction algorithms, recently proposed multipass whole-body (WB) protocols in conjunction with image-derived input functions (IF) have made WB kinetic parameter estimation feasible [2]. Here we present a case of a patient with bronchial cancer and a venous thrombus in the left brachiocephalic vein (green arrows) with unclear FDG accumulation in the left axillary region (blue arrows) on

SUV images (a). The patient was injected (134.1 MBq) and data over the heart were acquired for 7 min (blue insert: 155–180 s), followed by 10 WB passes (35 s/bed). The IF was extracted from the descending aorta and after appropriate corrections was used to estimate glucose influx (Ki) (b) and volume of distribution (Vd) (c) [3]. Note the high tumor uptake (red arrows) while missing accumulation in the axillary region on Ki (b), compared to high uptake in venous regions but low accumulation in the primary tumor on Vd (c). Standard static imaging was performed after the WB dynamic protocol (2.5 min/bed) (a), axial images are given for both areas of interest (a1/a2, scaled SUV 0–6). Only after review of the parametric images, the cause of FDG accumulation was linked to venous collaterals due to thrombosis.


This article is part of the Topical Collection on Oncology - Chest.

✉ Irene A. Burger
irene.burger@usz.ch

¹ Department of Nuclear Medicine, University Hospital Zurich, University of Zurich, Rämistrasse 100, 8091 Zürich, Switzerland

² GE Healthcare, Waukesha, WI, USA

³ Department of Nuclear Medicine, Cantonal Hospital of Baden, Baden, Switzerland

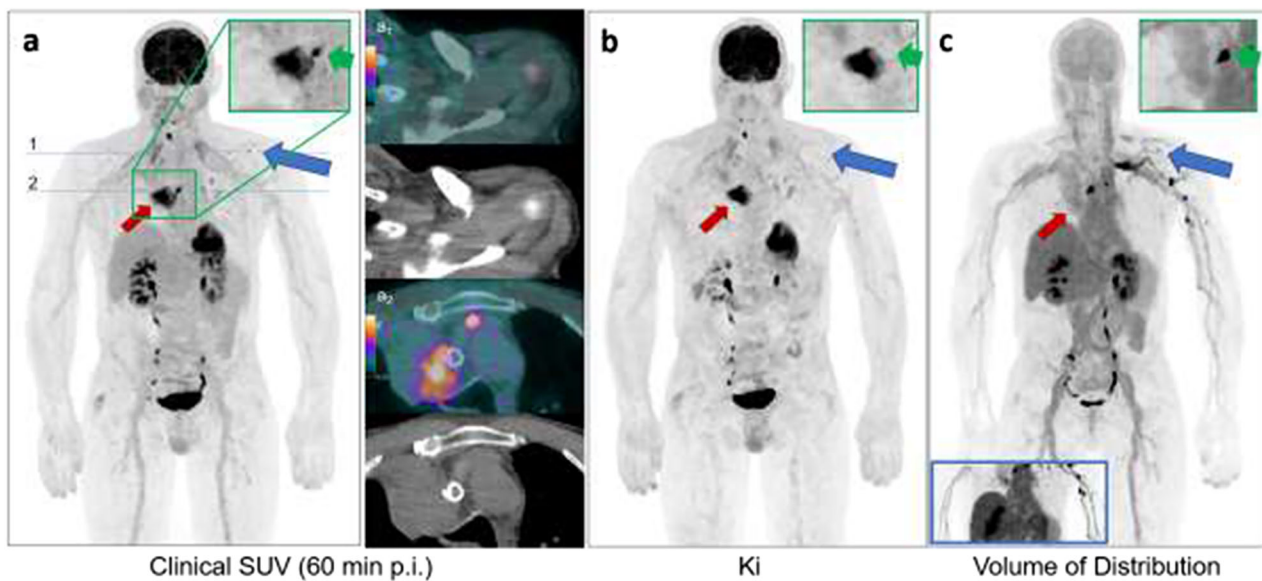

Acknowledgements Open Access funding provided by Universität Zürich.

Funding The Nuclear Medicine Department holds GE grants.

Compliance with ethical standards

Conflict of interest F.K. is an employee of GE imaging. He was involved in image reconstruction, not in image interpretation. I.A.B. and M.H. have received research grants and speaker honoraria from GE. All other authors declare that they have no conflict of interest.

Ethics approval Ethics approval and informed consent was given.

Open Access This article is licensed under a Creative Commons Attribution 4.0 International License, which permits use, sharing, adaptation, distribution and reproduction in any medium or format, as long as you give appropriate credit to the original author(s) and the source, provide a link to the Creative Commons licence, and indicate if changes were made. The images or other third party material in this article are included in the article's Creative Commons licence, unless indicated otherwise in a credit line to the material. If material is not included in the article's Creative Commons licence and your intended use is not permitted by

statutory regulation or exceeds the permitted use, you will need to obtain permission directly from the copyright holder. To view a copy of this licence, visit <http://creativecommons.org/licenses/by/4.0/>.

References

1. Nanette MT. Freedman et al Comparison of SUV and Patlak slope for monitoring of cancer therapy using serial PET scans. *Eur J Nucl Med*. 2003;30:46–53.
2. Karakatsanis NA, Lodge MA, Tahari AK, Zhou Y, Wahl RL, Rahmim A. Dynamic whole-body PET parametric imaging: I. Concept, acquisition protocol optimization and clinical application. *Phys Med Biol*. 2013;58(20):7391–418. <https://doi.org/10.1088/0031-9155/58/20/7391>.
3. Patlak C, Blasberg R. Graphical evaluation of blood-to-brain transfer constants from multiple-time uptake data. Generalizations. *J Cereb Blood Flow Metab*. 1985;5:584–90.

Publisher's note Springer Nature remains neutral with regard to jurisdictional claims in published maps and institutional affiliations.